

Inertsil ODS-EP Technical Information


Advantages of Inertsil ODS-EP

- The selectivity is completely different from those of conventional columns such as ODS column due to its specific polar group in the stationary phase.
- Durability can be obtained by the high density bonding.
- Superior peak shapes of both acids and bases can be obtained because of neutral bonded phase and low residual silanol groups.
- Silica gel of high-purity is used as the support material, which minimizes effects of any remaining metal ions.
- Specifications of Inertsil ODS-EP

	Support Silica Gel					Chemical Modification	
	Partical diameter	Shape	Specific surface area	Pore diameter	Purity	Bonded group	ODS Carbon content
Inertsil ODS-EP	5 μ m	Spherical	450m ² /g	100Å	99.999	Embeddedpolar Octadecyl group	9 %

(1) Naphthalene sample

~ for measurement retention and peak shape ~

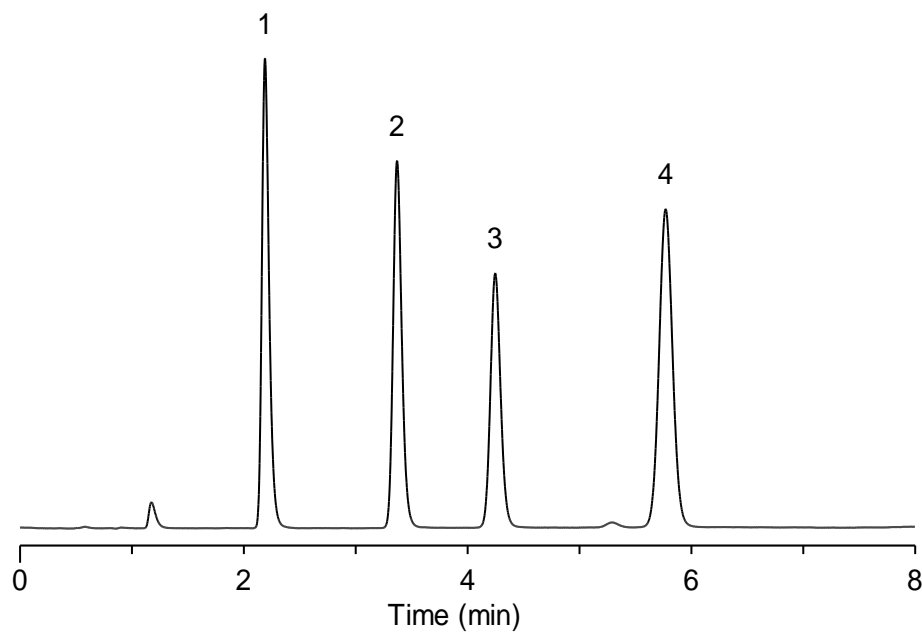

Inertsil ODS-EP

Conditions

Column dimensions:

4.6 mm I.D x 150 mm length

Mobile phase:

Acetonitrile : Water =65 : 35

Flow rate: 1 ml / min







Column temperature: 40°C

Detection: UV 254 nm






Peak identification

1. Acetophenone
2. Benzene
3. Toluene
4. Naphthalene


Comparison of retention between Inertsil ODS-EP and commercial embedded columns

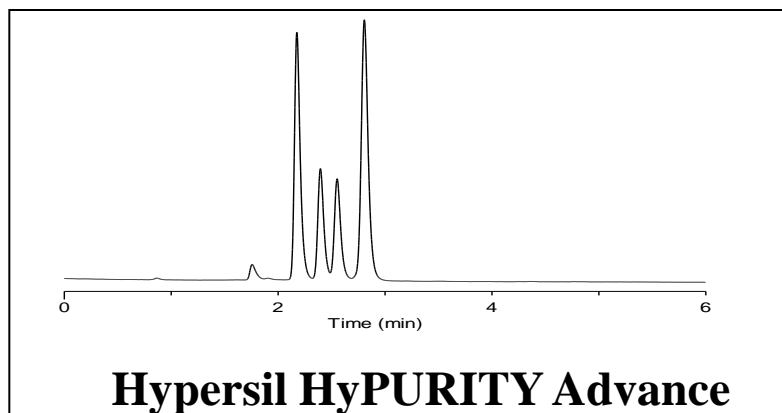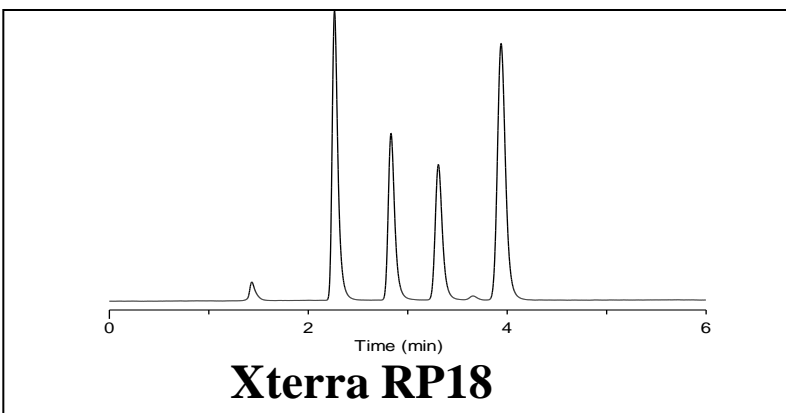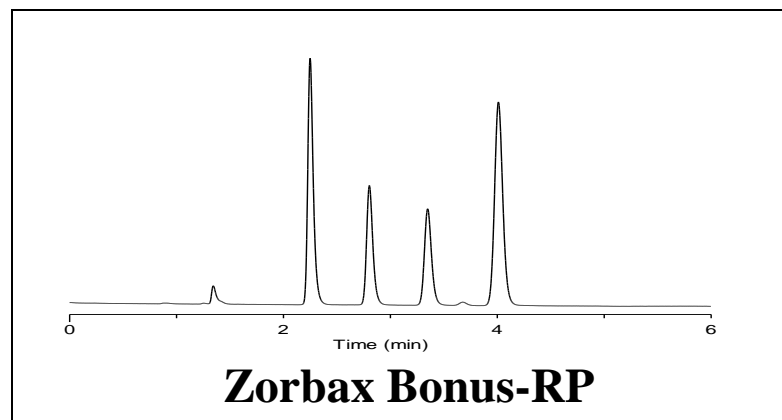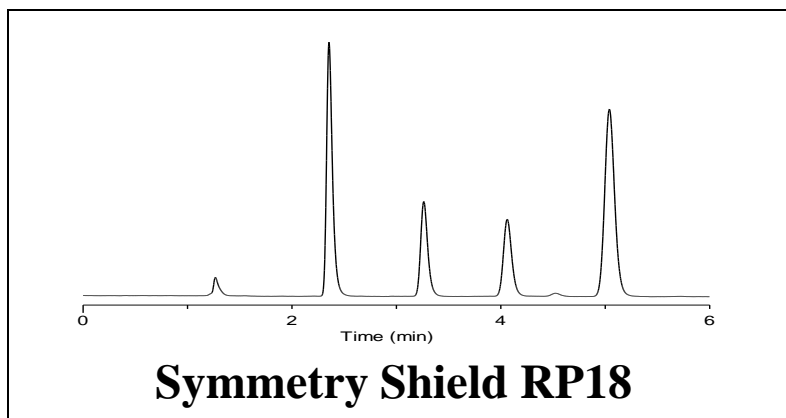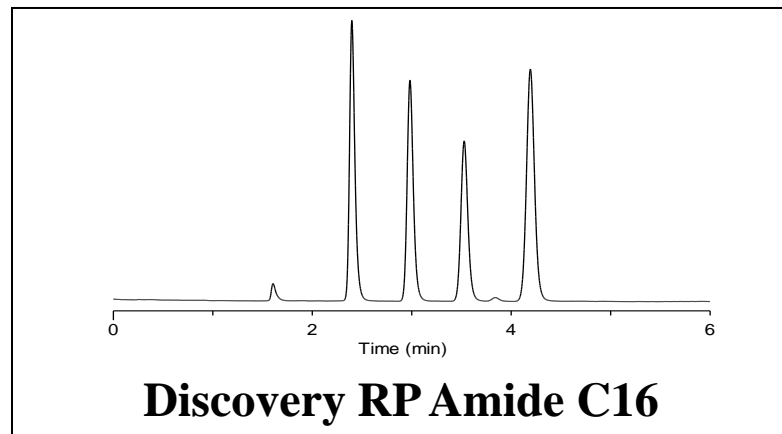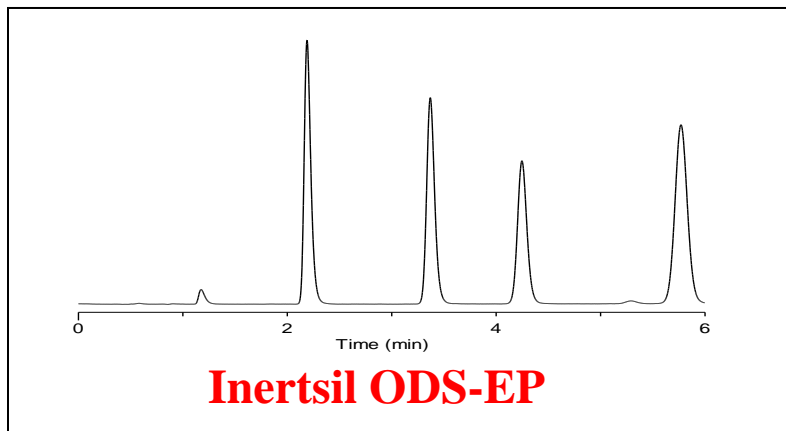

Comparison of retention between Inertsil ODS-EP and other type commercial columns

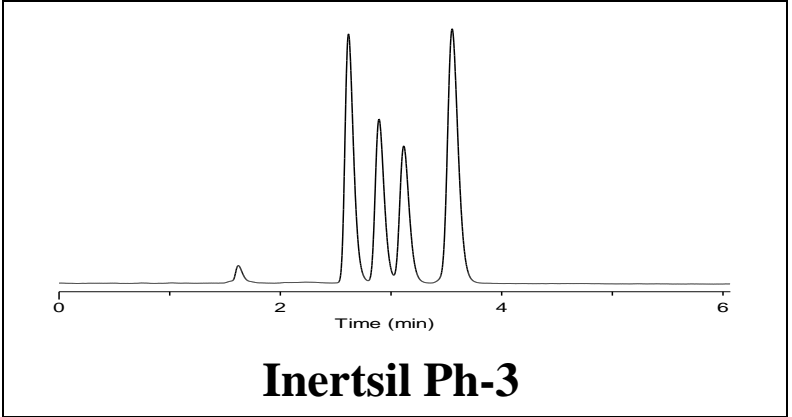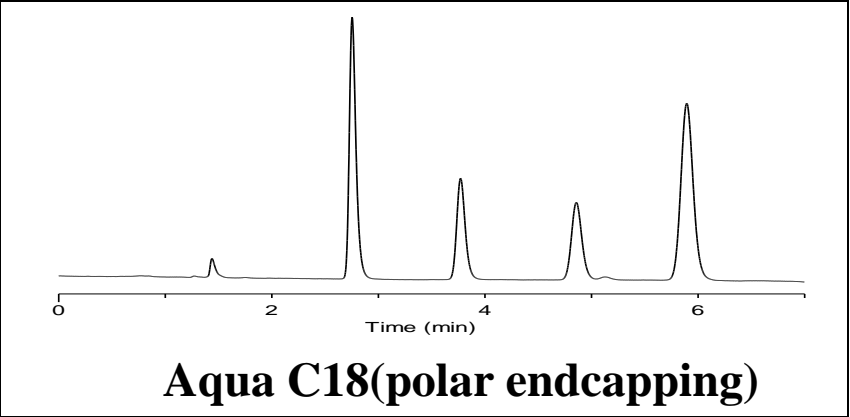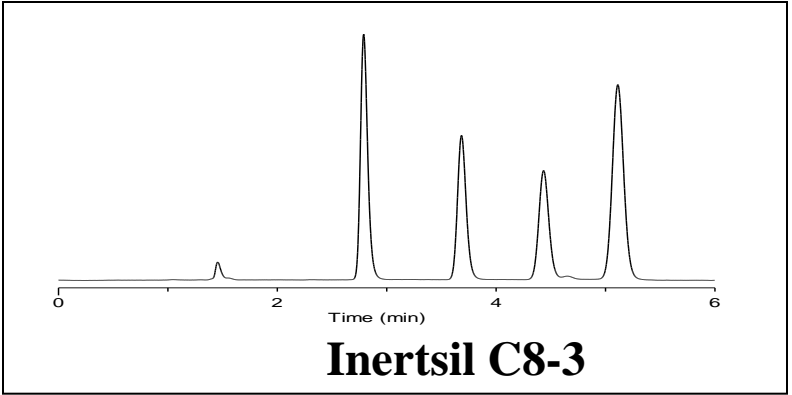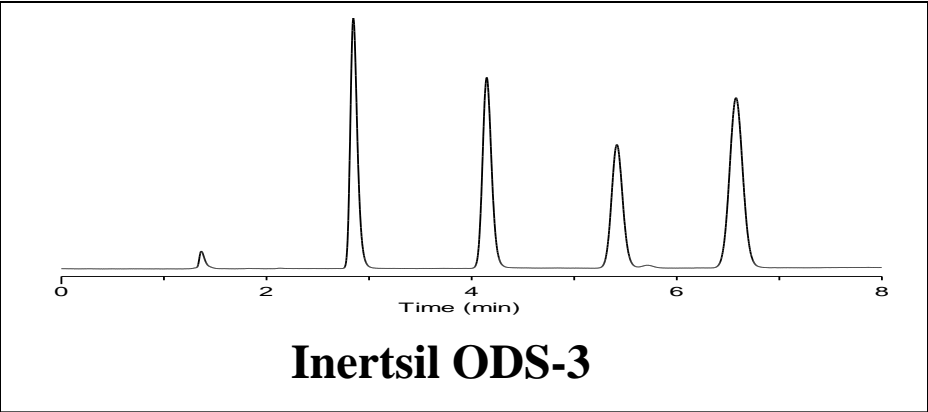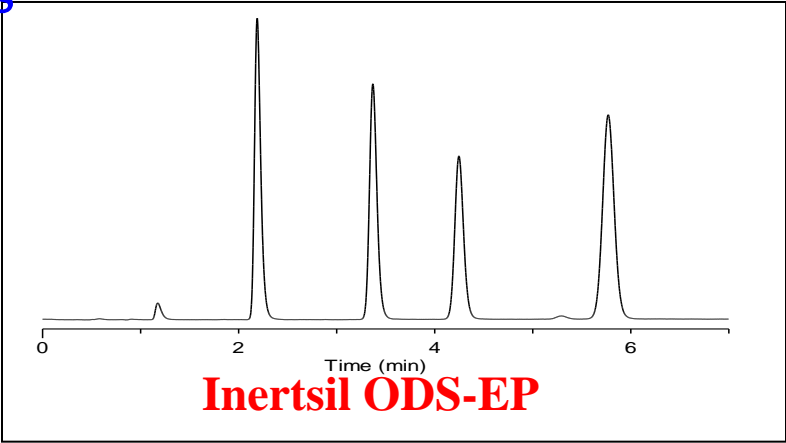

(2) Selectivity test sample ~ for measurement selectivity ~

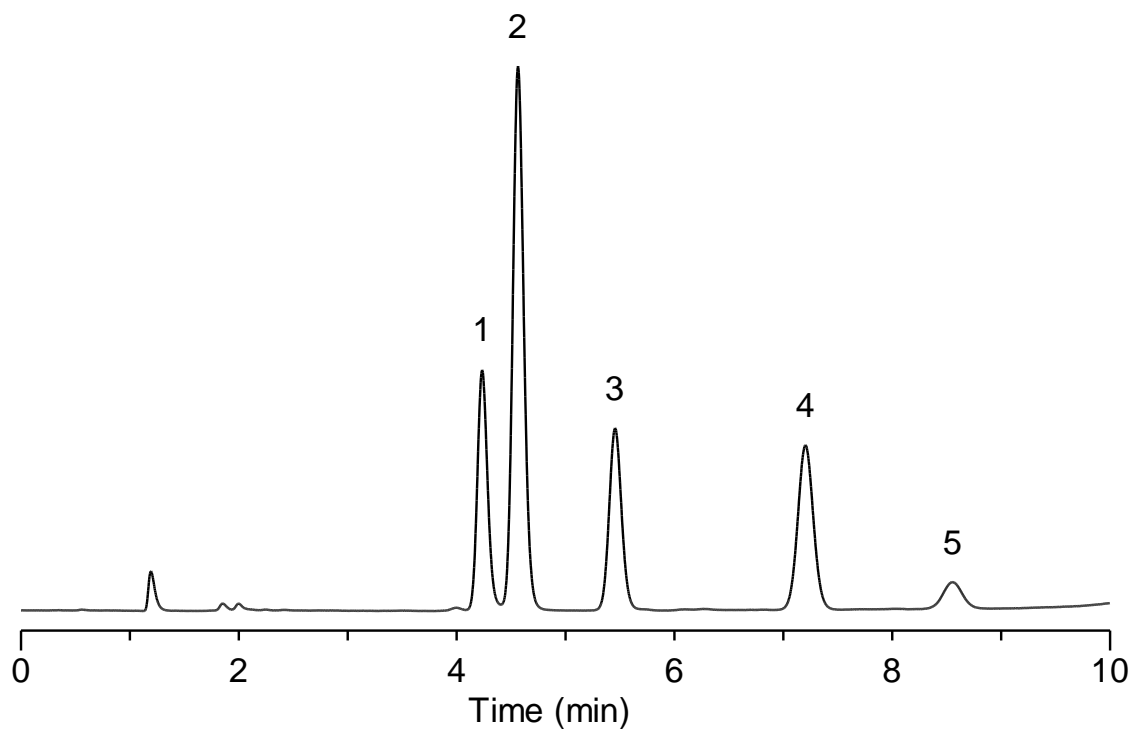

Inertsil ODS-EP

Conditions

Column dimensions:

4.6 mm I.D x 150 mm length

Mobile phase:

Acetonitrile : Water = 70 : 30


Flow rate: 1 ml / min

Column temperature: 40°C


Detection: UV 265 nm

Peak identification


1. Ethylbenzene




2. Naphthalene




3. n-Propylbenzene









4. n-Butylbenzene








5. Anthracene




Comparison of selectivity between Inertsil ODS-EP and commercial embedded columns

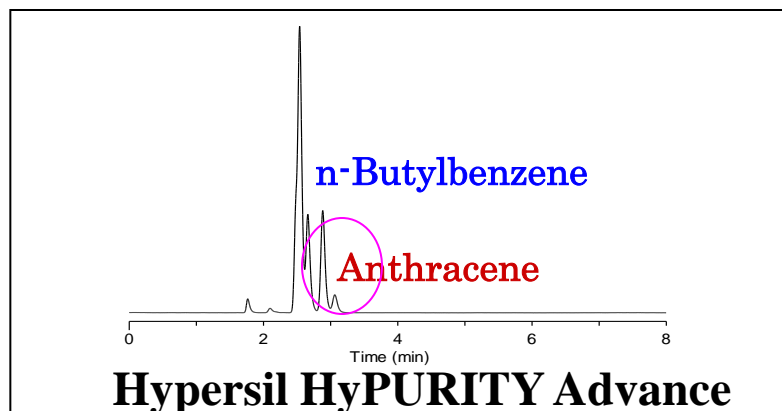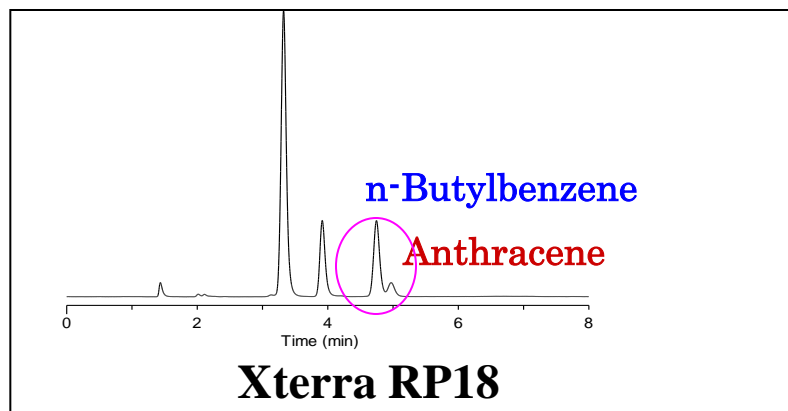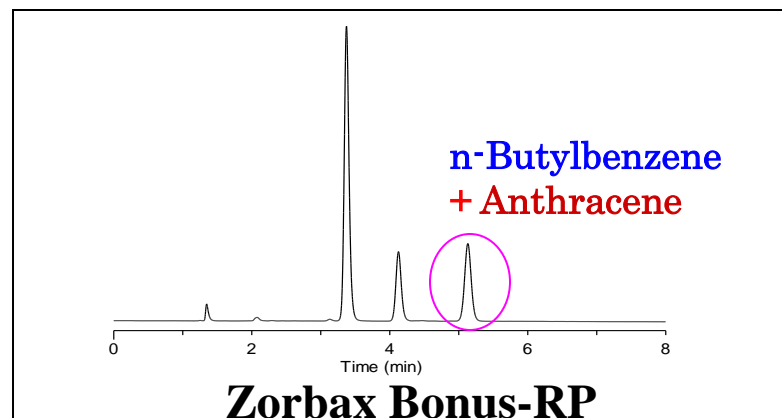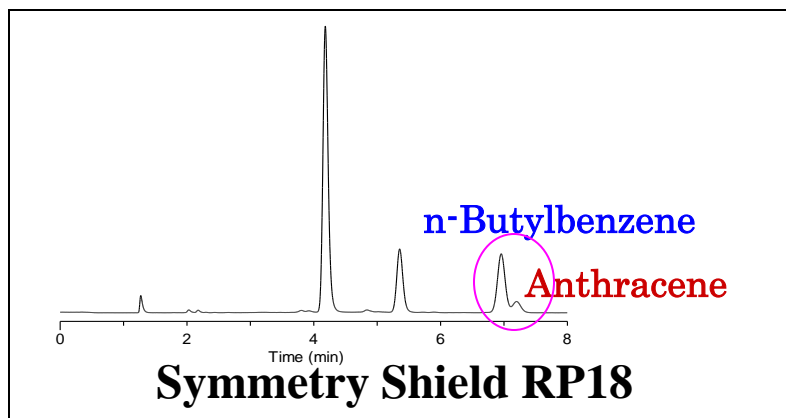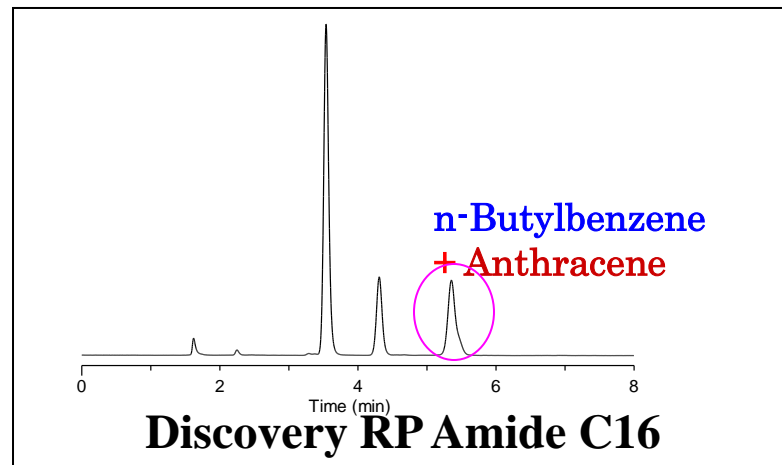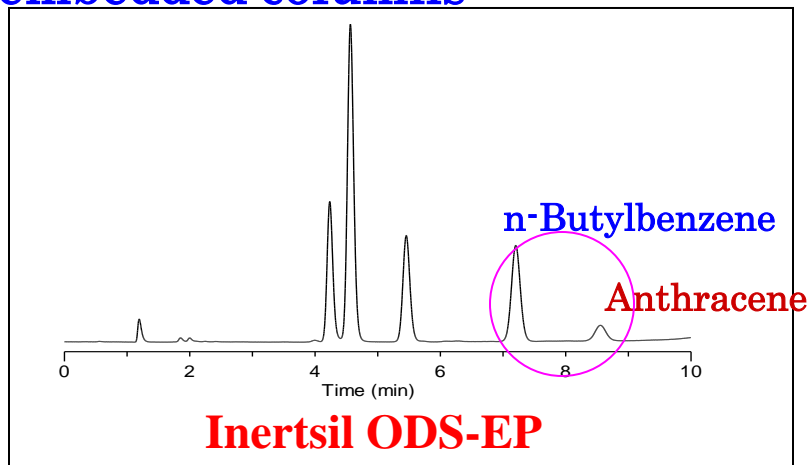

Comparison of selectivity between Inertsil ODS-EP and other type commercial columns

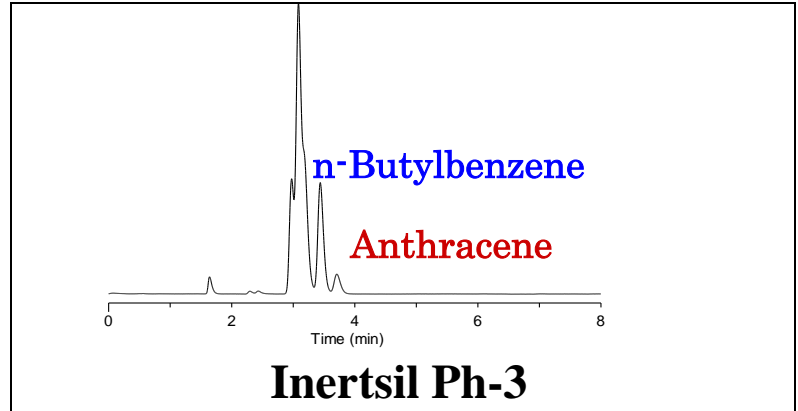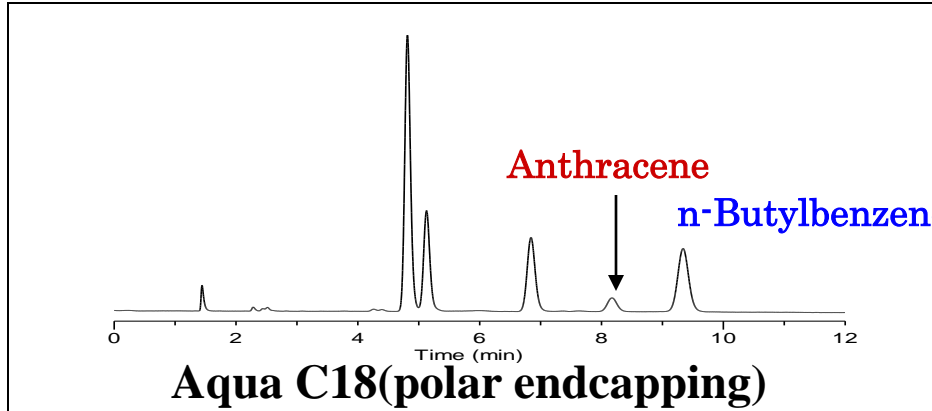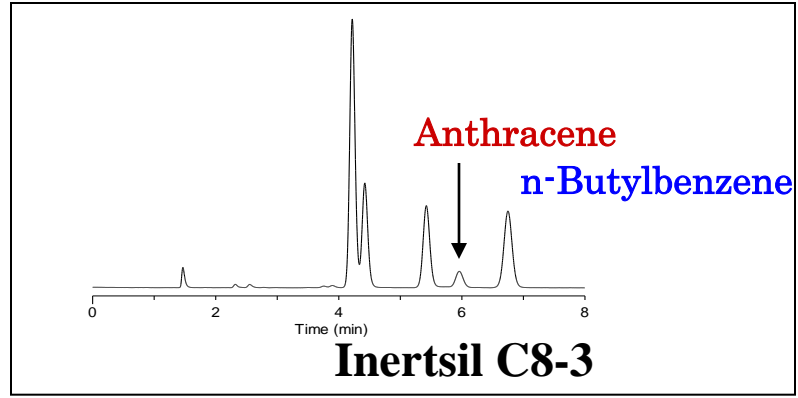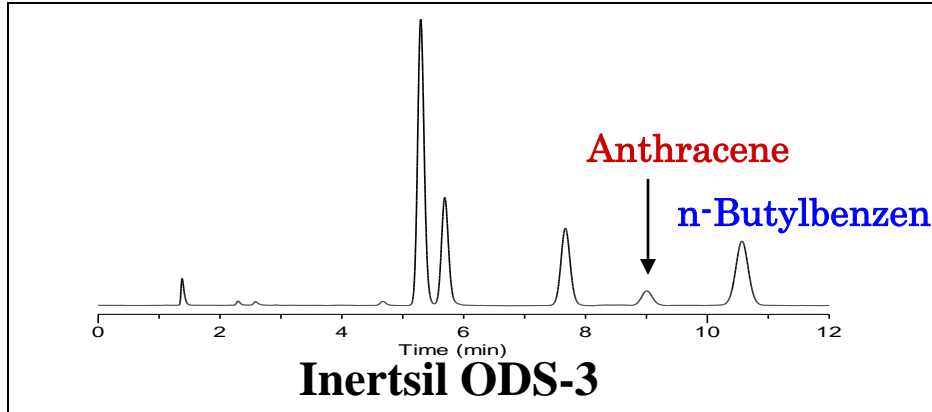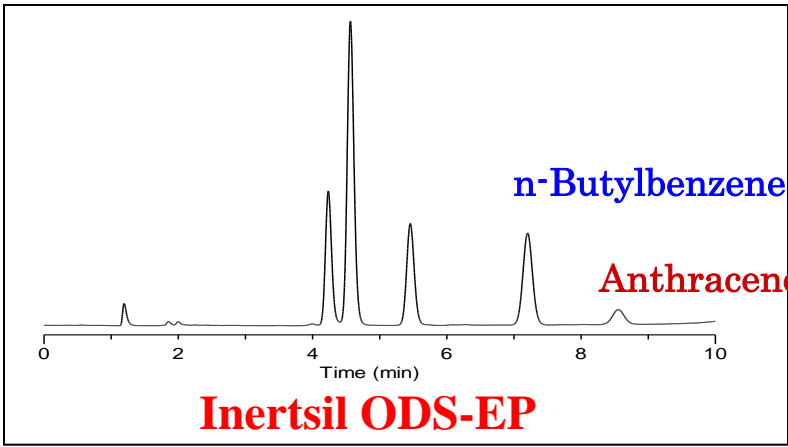


Comparison of retention and selectivity between Inertsil ODS-EP and commercial embedded columns

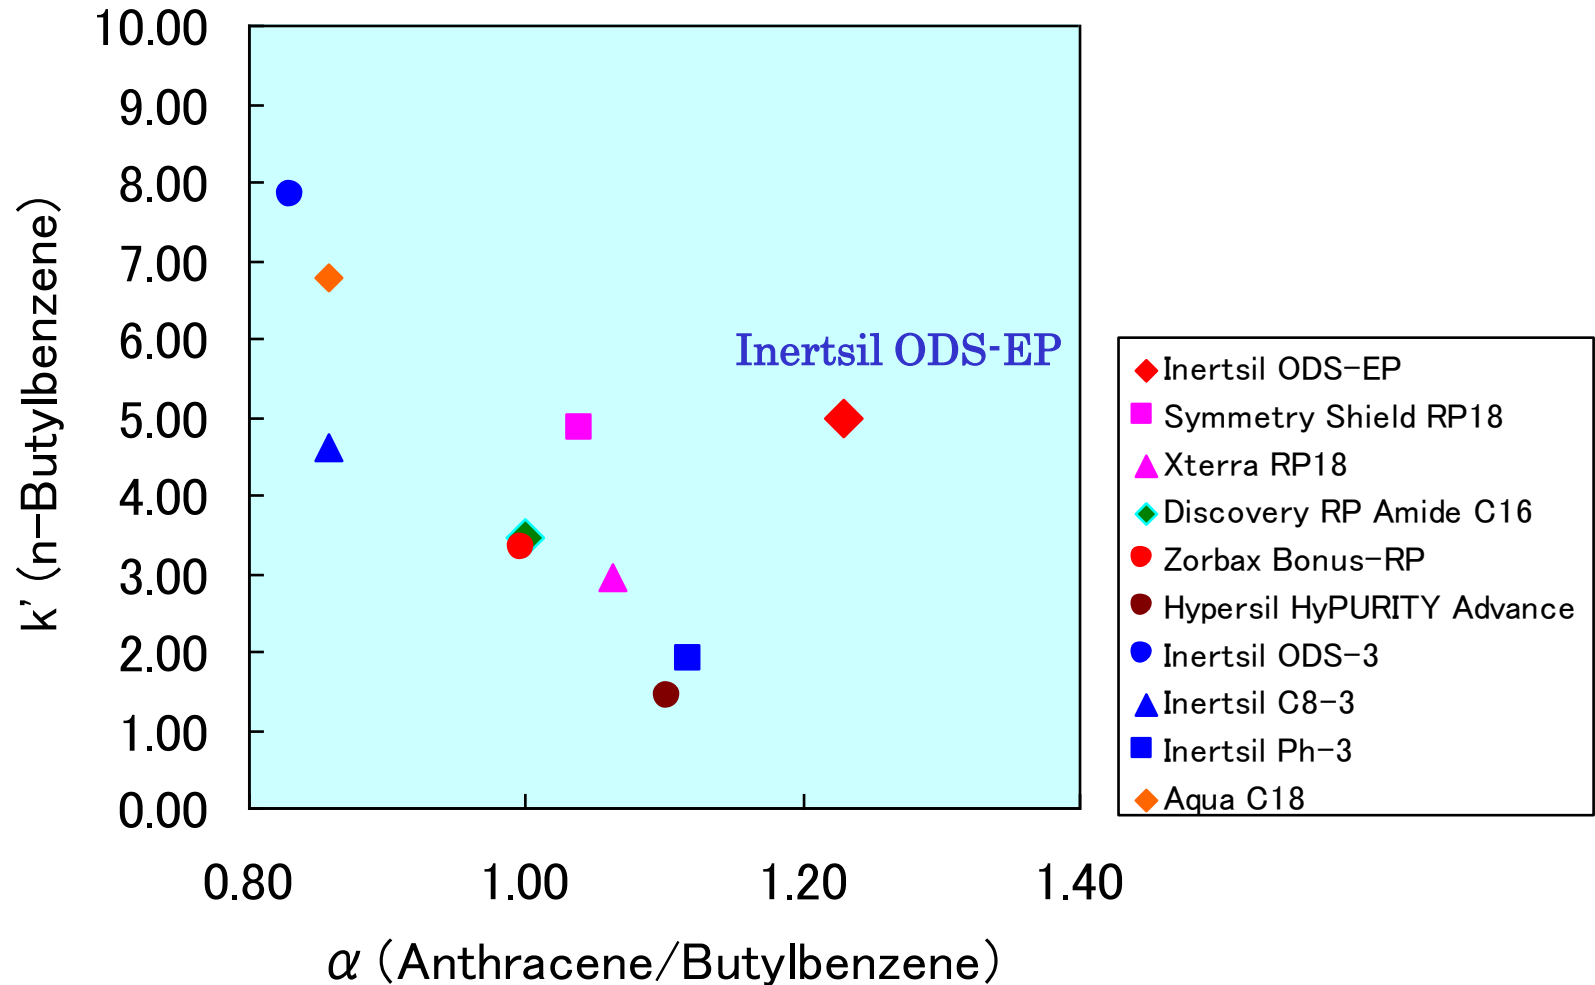

The selectivity of Inertsil ODS-EP is completely different from those of conventional columns such as ODS column due to its specific polar group in the bonded phase.

(3) Tanaka-test sample

~ for measurement selectivity, hydrogen bonding capacity and hydrophobicity ~

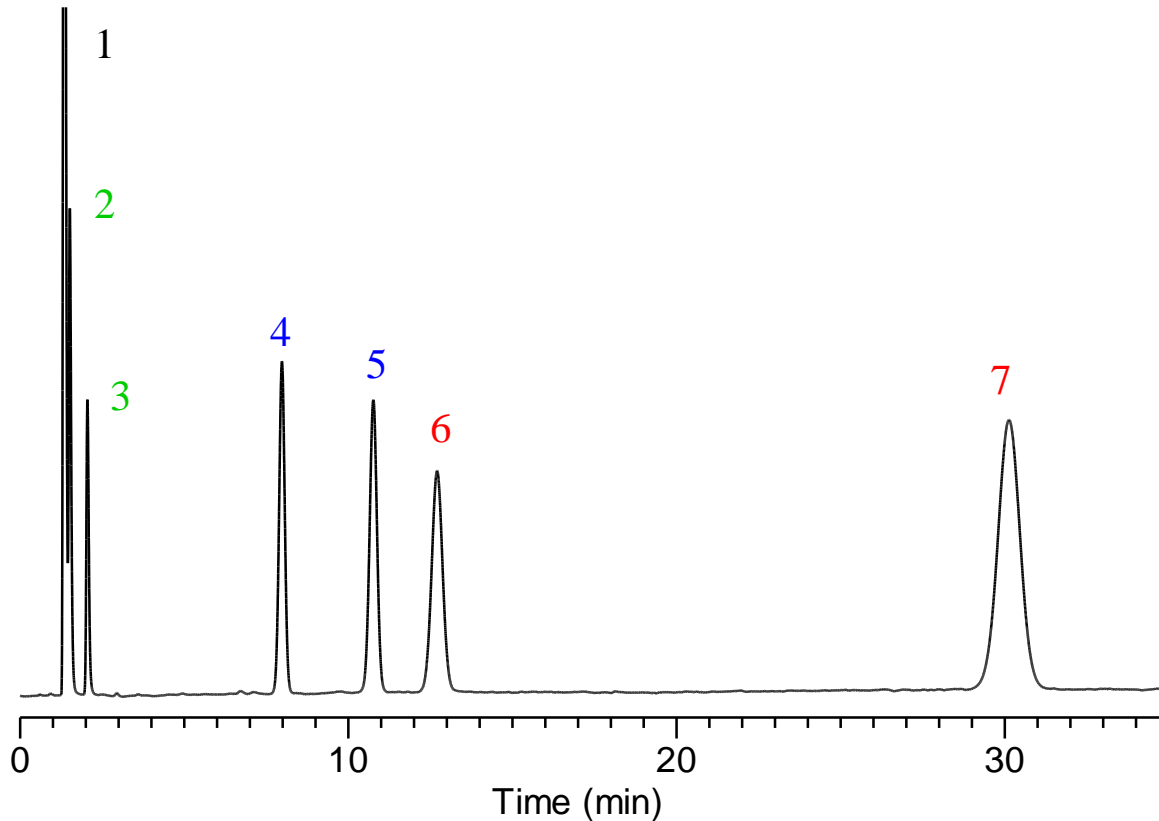

Inertsil ODS-EP

Conditions

Column dimensions:

4.6 mm I.D x 150 mm length

Mobile phase:

Methanol : Water = 80 : 20

Flow rate: 1 ml / min

Column temperature: 40°C

Detection: UV 254 nm

Peak identification

1. Uracil

2. Caffeine

3. Phenol







4. n-Butylbenzene

5. n-Amylbenzene






6. o-Terphenyl

7. Triphenylene

Comparison of selectivity between Inertsil ODS-EP and commercial embedded columns

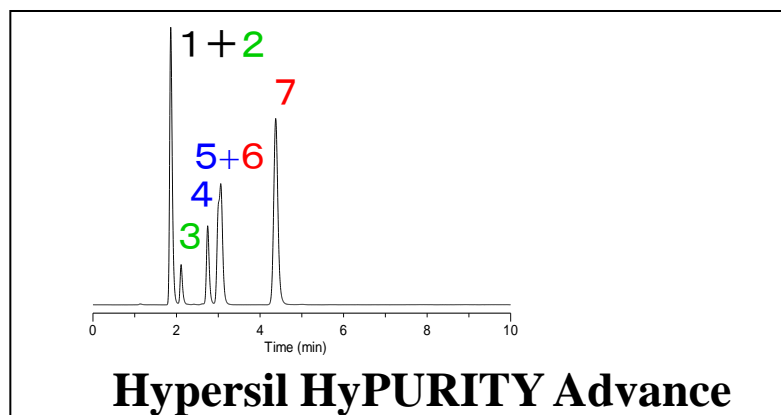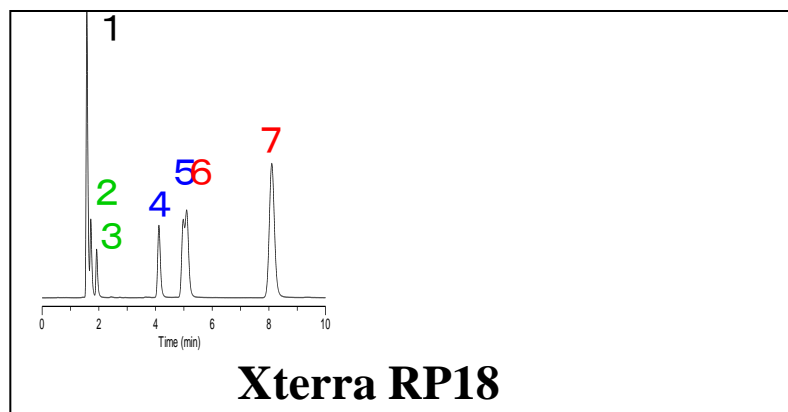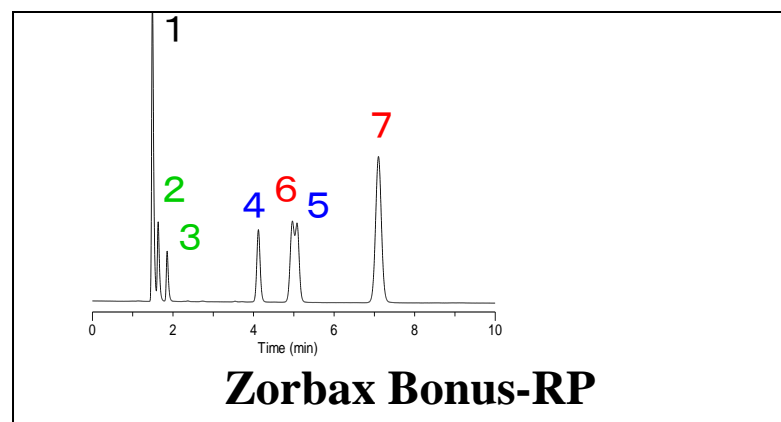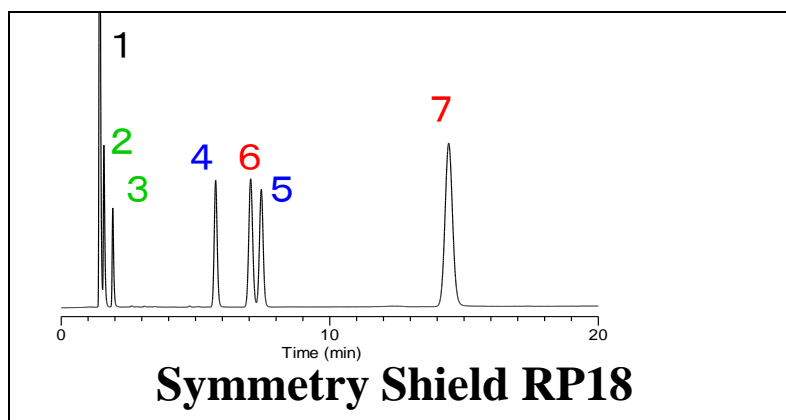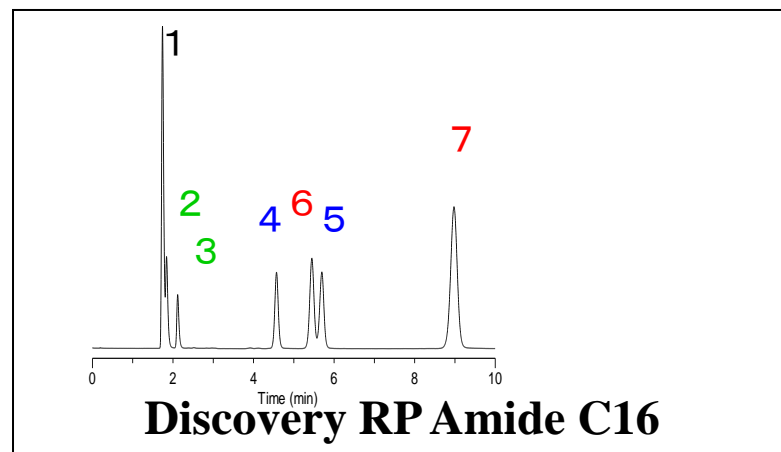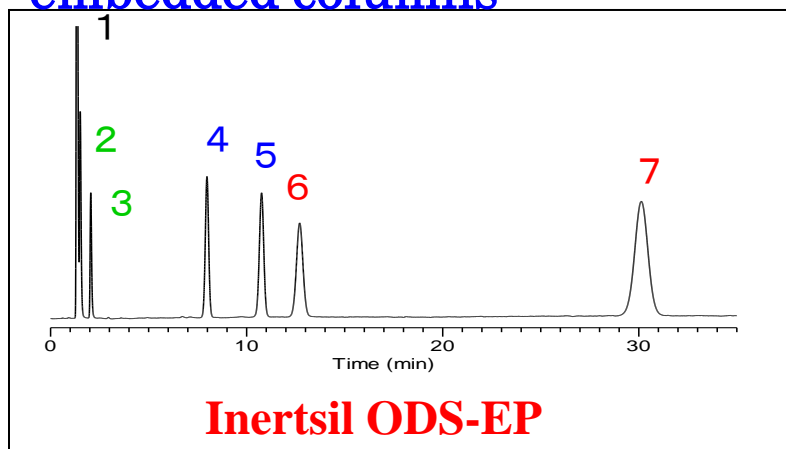


Comparison of selectivity between Inertsil ODS-EP and other type commercial columns

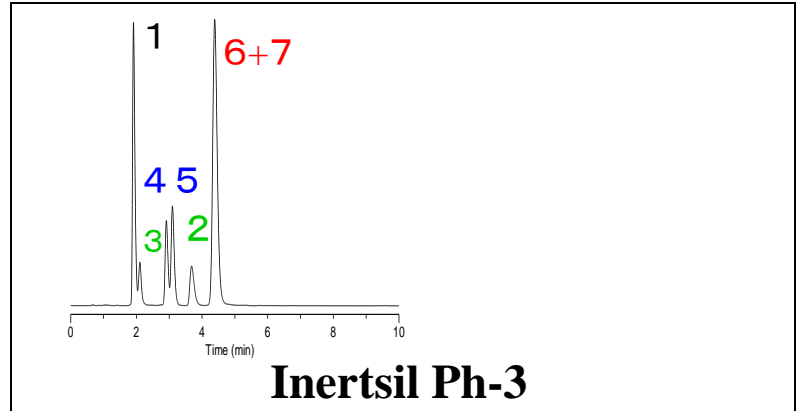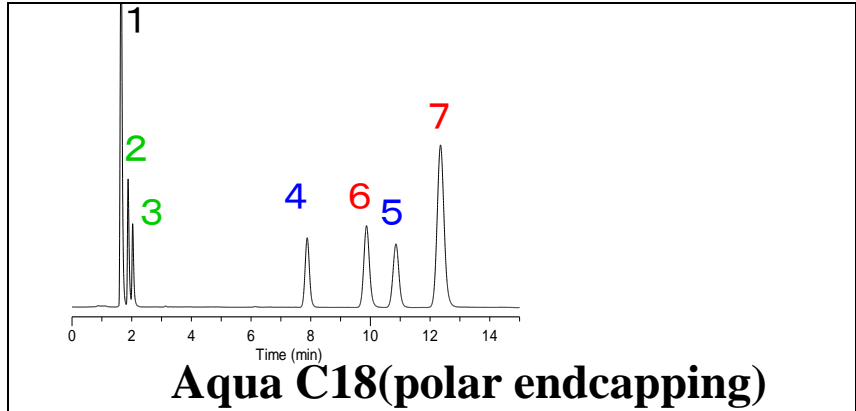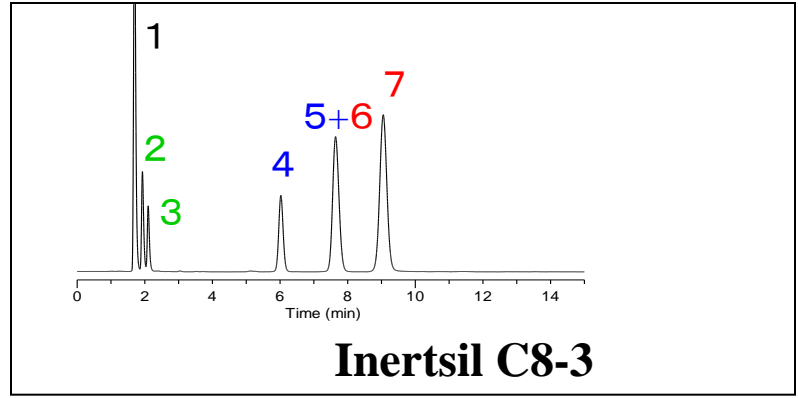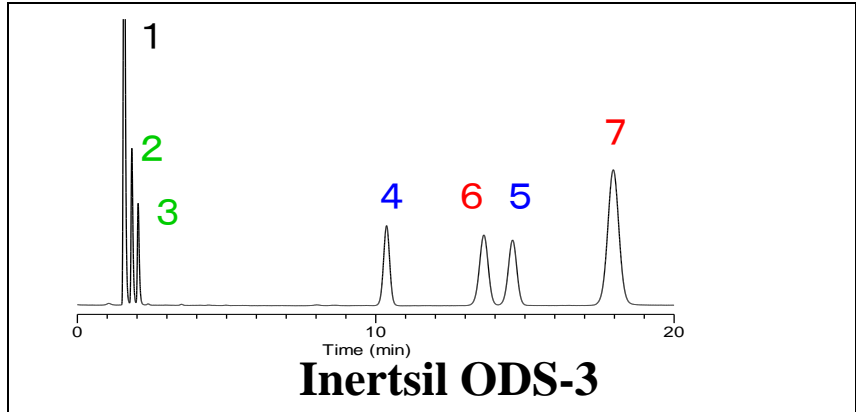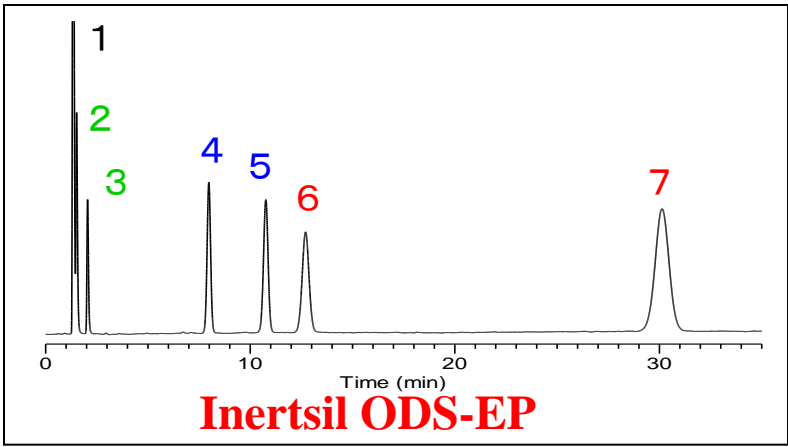


Characterization of Inertsil ODS-EP and commercial embedded columns by Tanaka test

Hydrogen bonding capacity

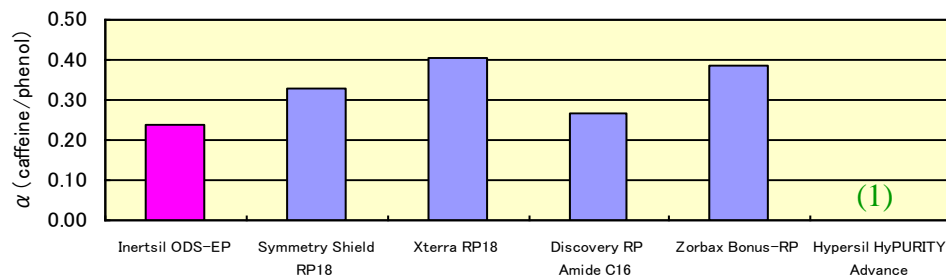


(1) Caffeine shows no retention

Hydrophobicity

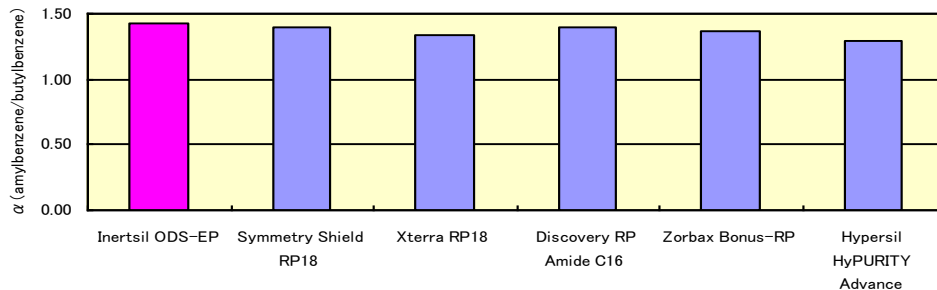

Steric selectivity

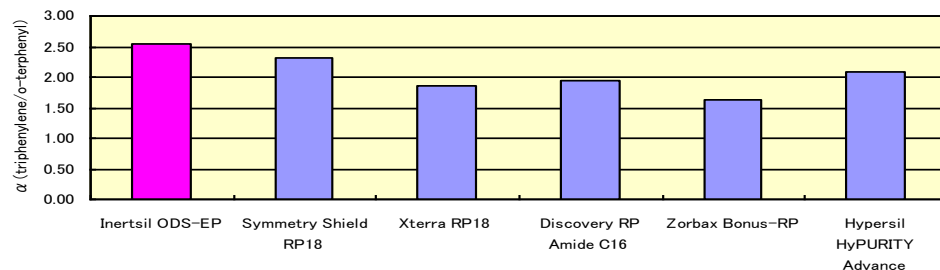

Conditions

Column dimensions:

4.6 mm I.D x 150 mm length


Mobile phase:

Methanol : Water = 80 : 20


Flow rate: 1 ml / min

Column temperature: 40°C


Detection: UV 254 nm




Caffeine




Phenol




n-Butylbenzene



n-Amylbenzene




o-Terphenyl



Triphenylene

(4) Pyridine-Phenol sample

~ for measurement of inertness to basic compounds ~

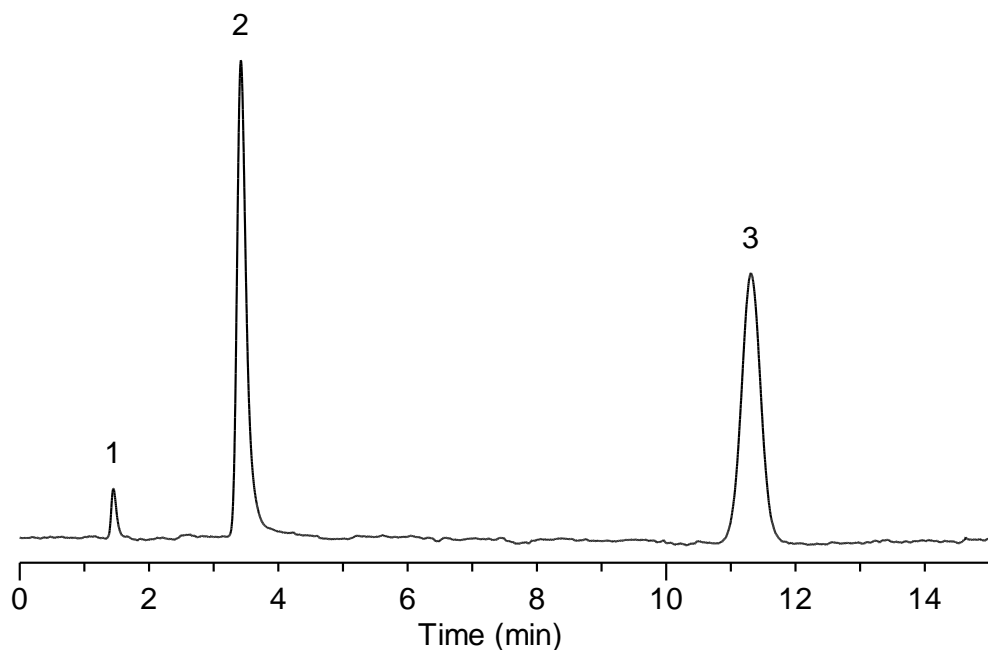

Inertsil ODS-EP

Conditions

Column dimensions:

4.6 mm I.D x 150 mm length

Mobile phase:

Methanol : 10mM Phosphate buffer(pH6.8)
=30 : 70

Flow rate: 1 ml / min

Column temperature: 40°C

Detection: UV 254 nm







Peak identification

1. Uracil

2. Pyridine


3. Phenol

Comparison of inertness to pyridine between Inertsil ODS-EP and commercial embedded columns

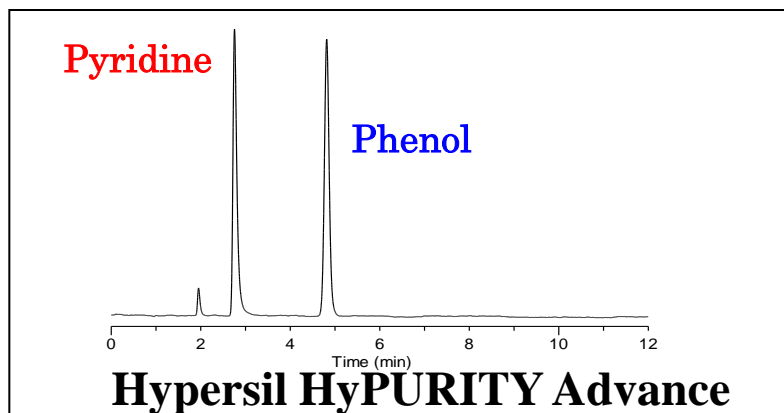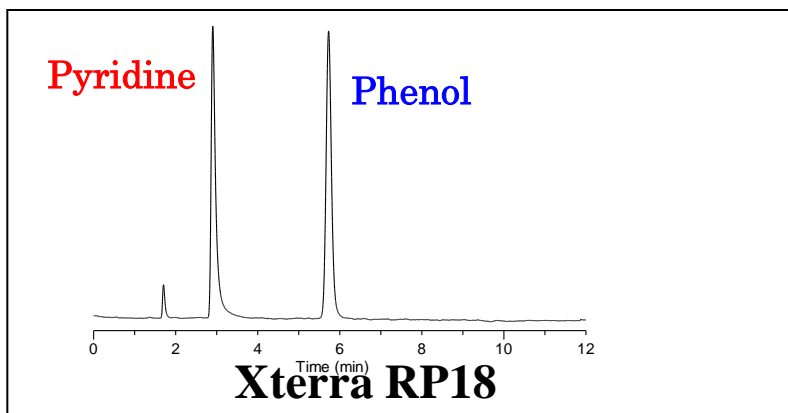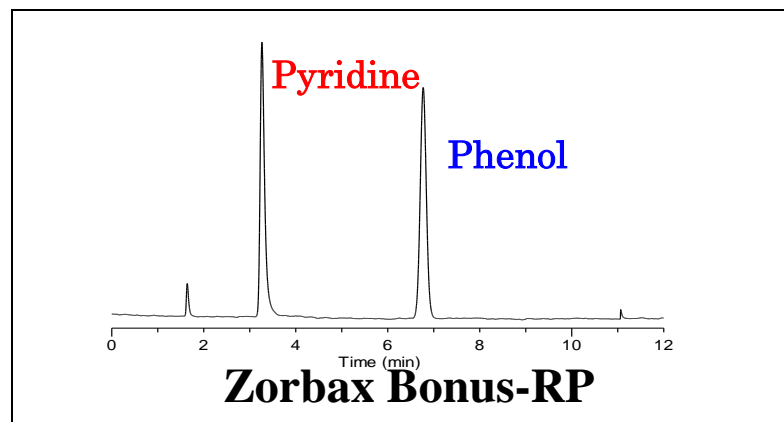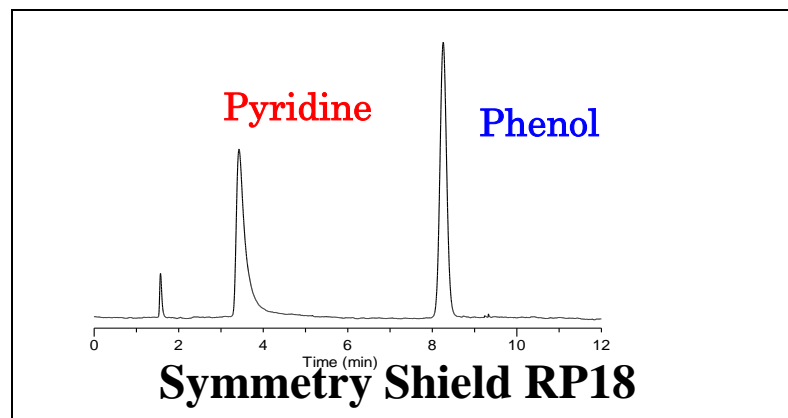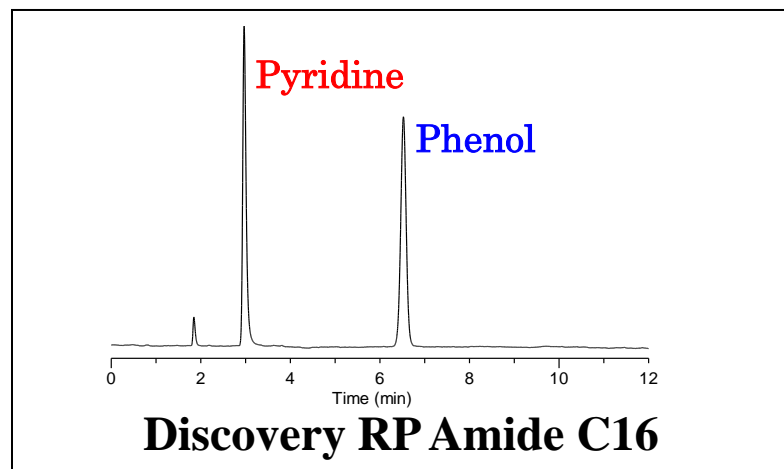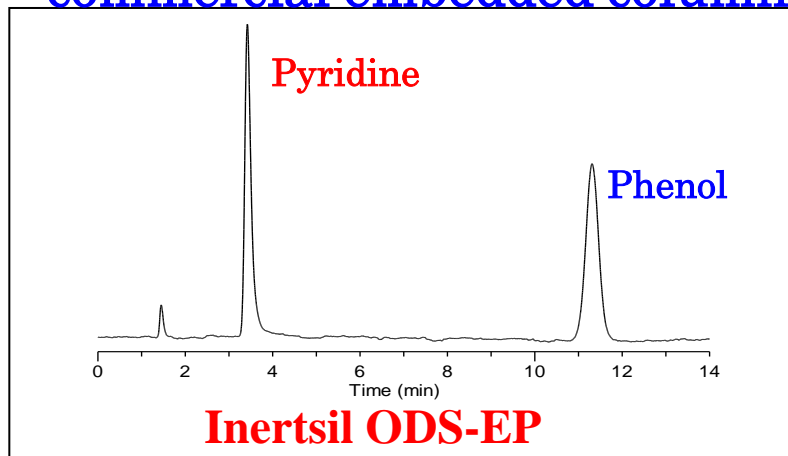

(5) Acid test sample

~ for measurement of inertness to acidic compounds ~

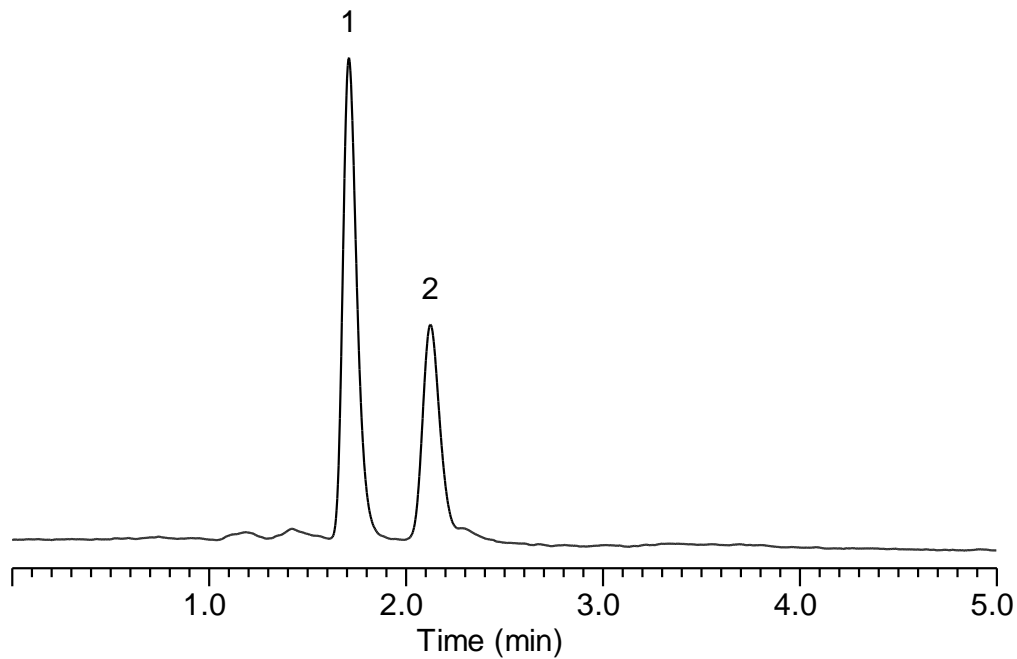

Inertsil ODS-EP

Conditions

Column dimensions:

4.6 mm I.D x 150 mm length

Mobile phase:

0.1% Phosphoric acid(pH2.2)

Flow rate: 1 ml / min

Column temperature: 40°C







Detection: UV 210 nm

Peak identification

1. Formic acid


2. Acetic acid

Comparison of inertness to acids between Inertsil ODS-EP and commercial embedded columns

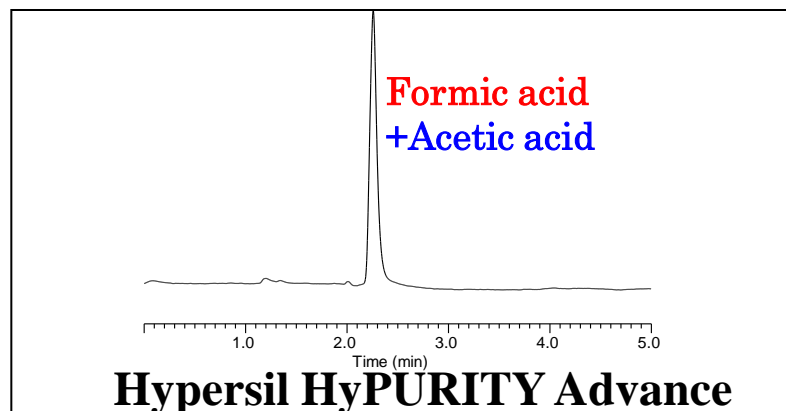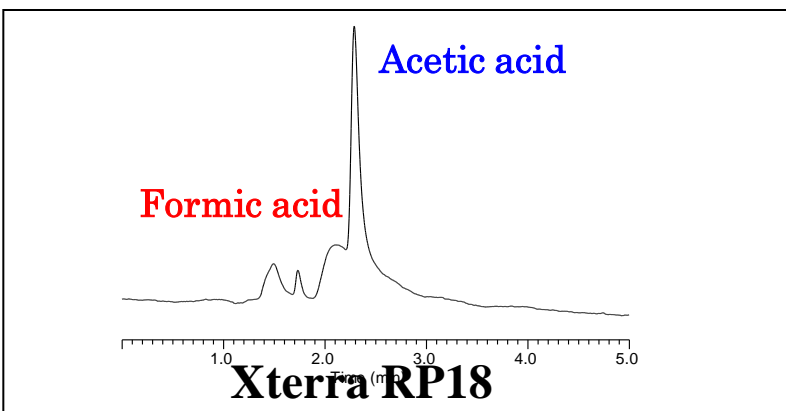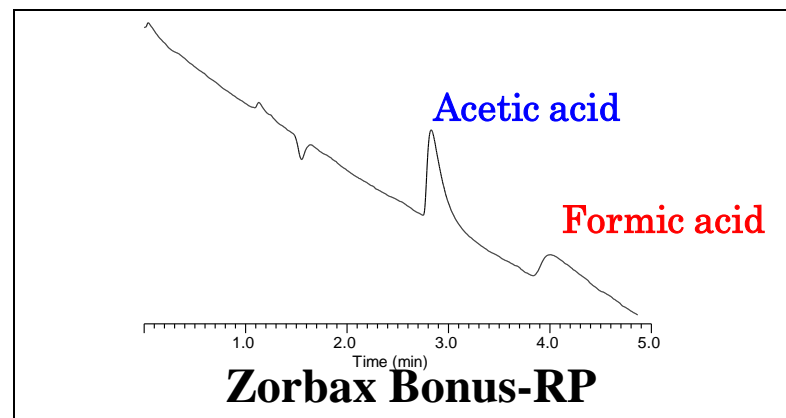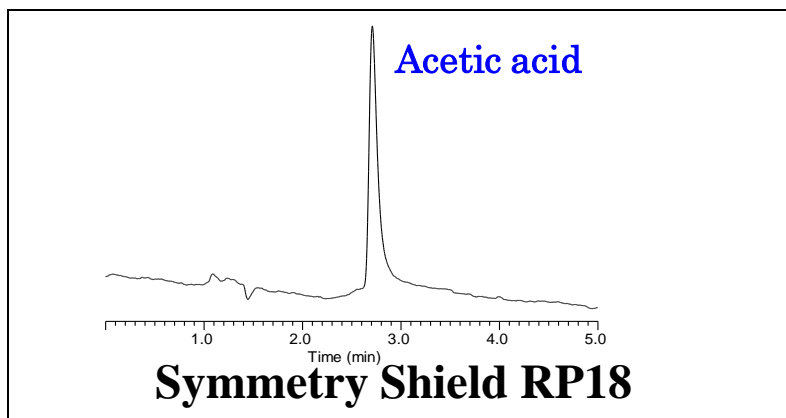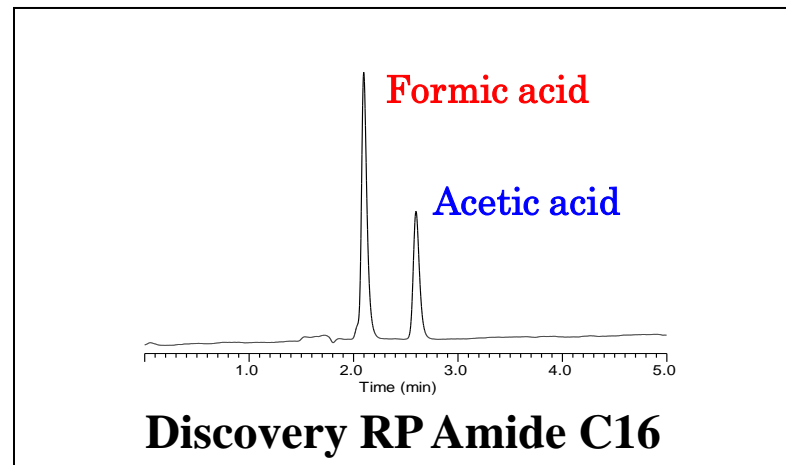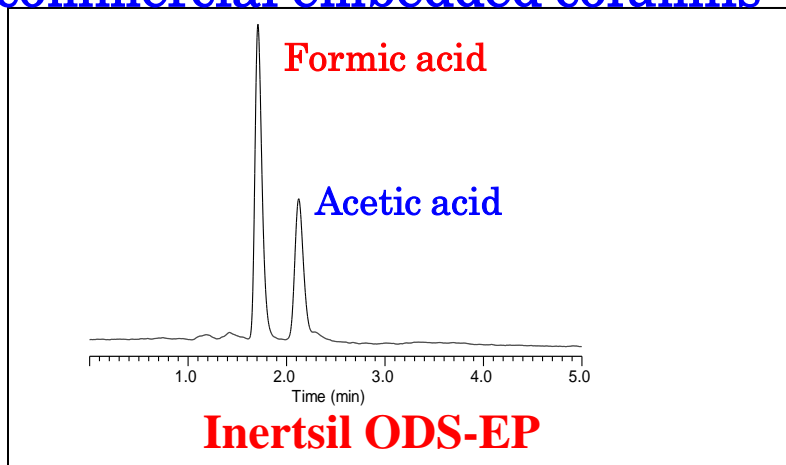

(6) Oxine-copper sample

~ for measurement of inertness to chelating compounds ~

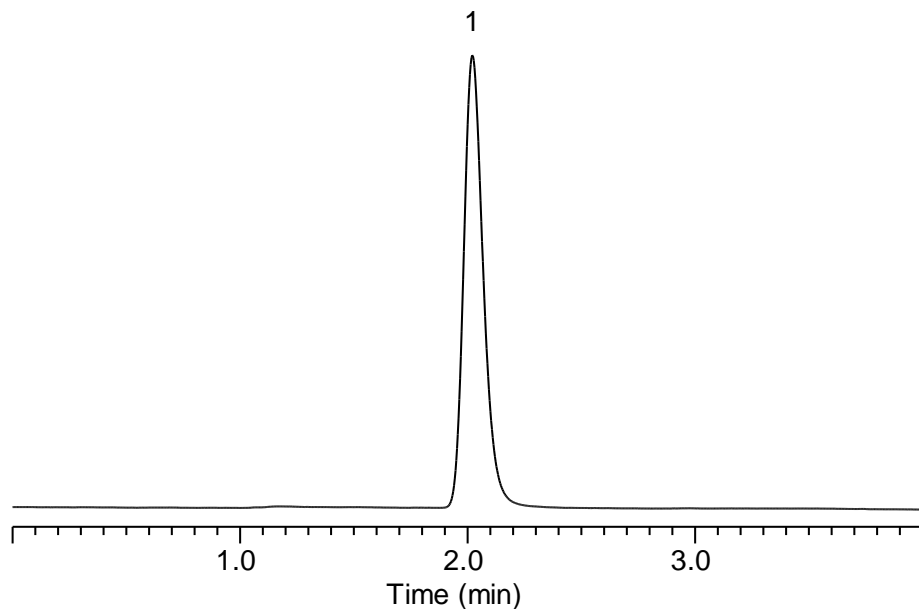

Inertsil ODS-EP

Conditions

Column dimensions:

4.6 mm I.D x 150 mm length

Mobile phase:

Acetonitrile : 0.1% Phosphoric acid(pH2.2)
=10 : 90

Flow rate: 1 ml / min







Column temperature: 40°C

Detection: UV 254 nm


Peak identification

1. Oxine-copper

Comparison of inertness to oxine-copper between Inertsil ODS-EP and commercial embedded columns

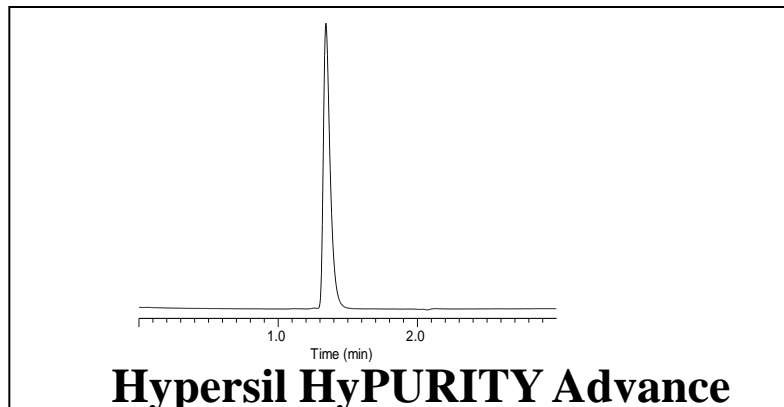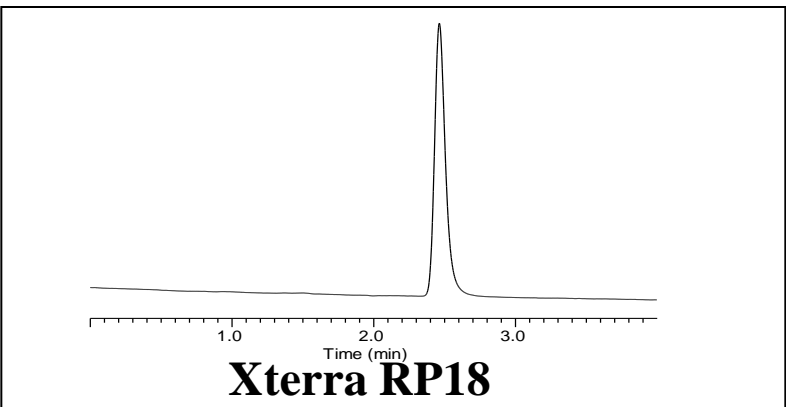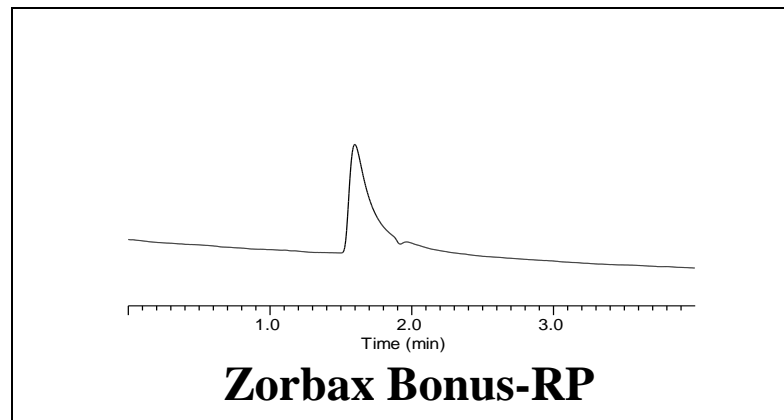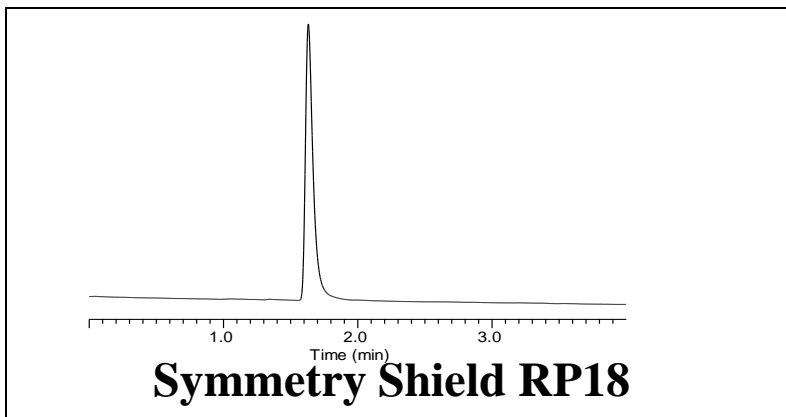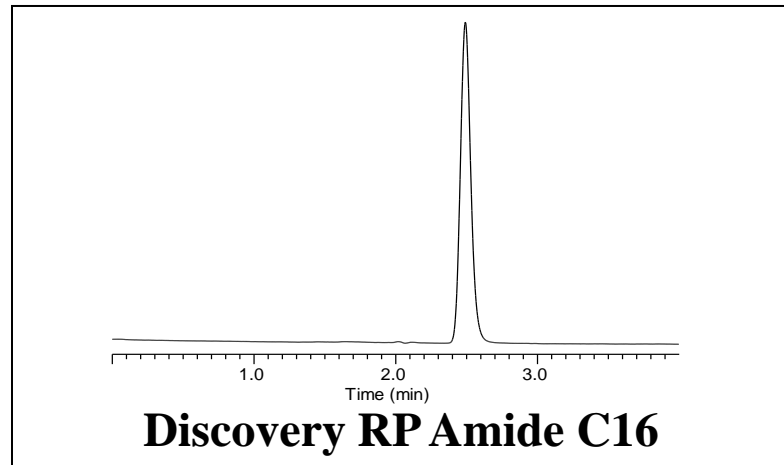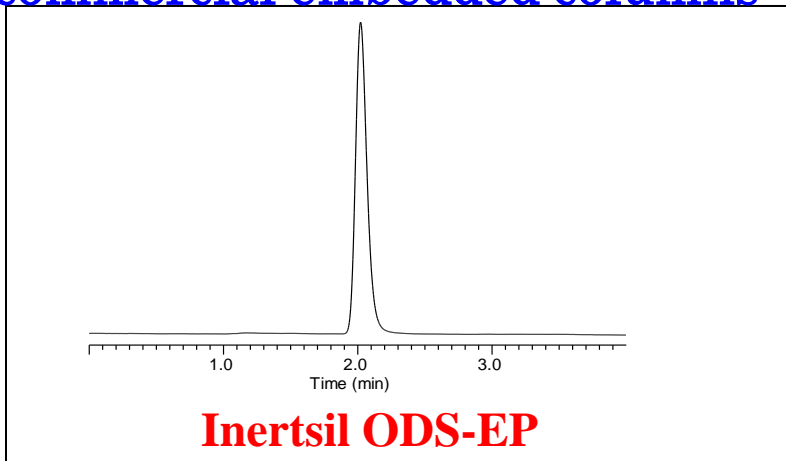

Comparison of durability among Inertsil ODS-EP, ODS column and Amide column

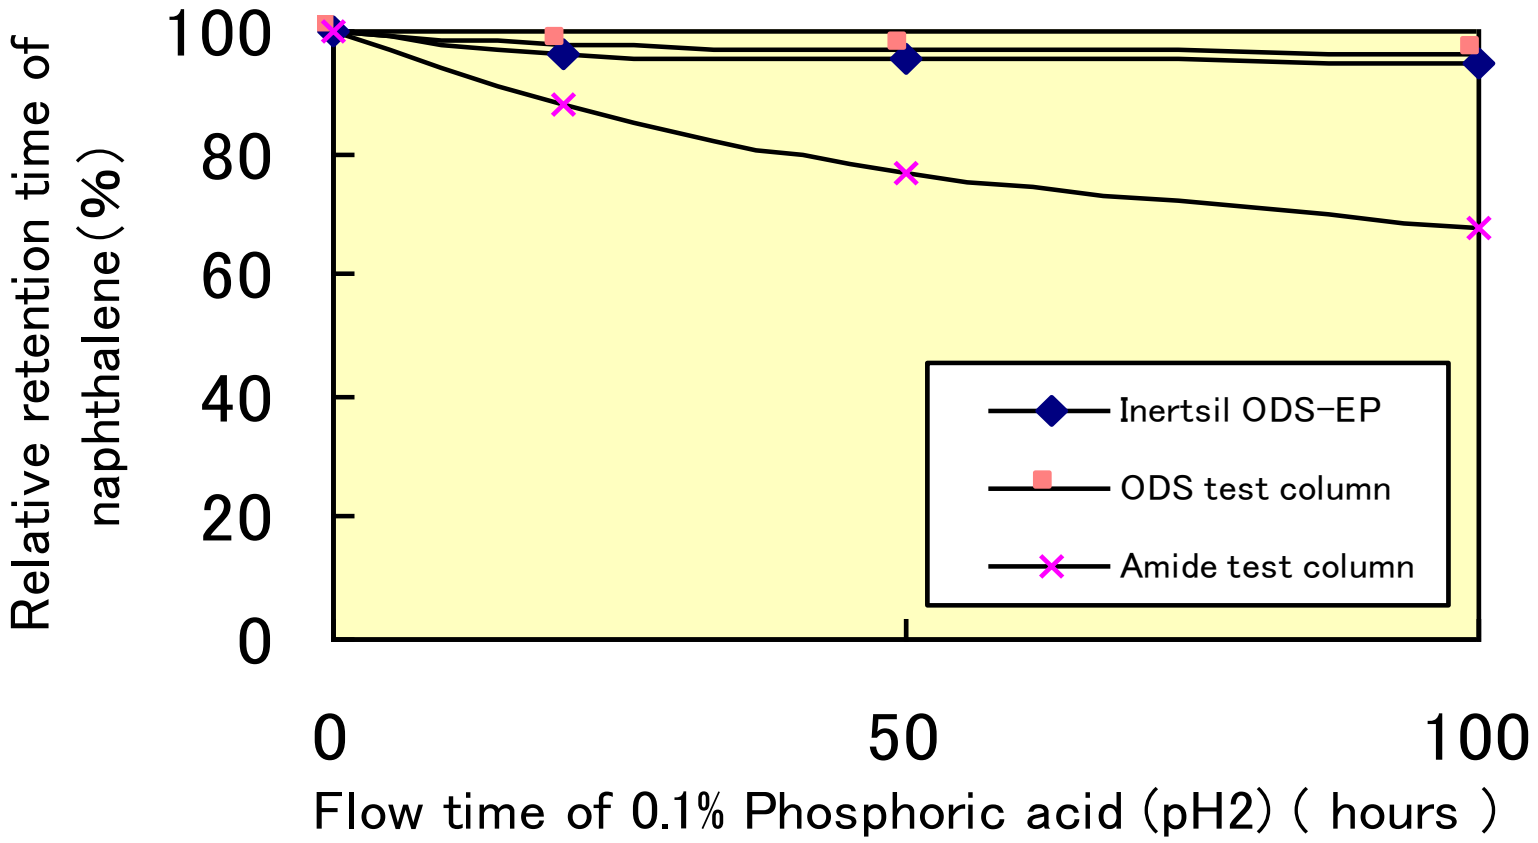

Test condition
Column: 4.6 mm I.D. x 150 mm
Flow rate: 1 ml / min
Column temperature: 30°C

Inertsil ODS-EP

- The selectivity is completely different from those of conventional columns such as ODS column, but the retention is close to conventional columns.

Inertsil ODS-EP is useful for the samples which are not separated by conventional columns.

- High durability can be obtained even if strong acid was used as mobile phase.

Inertsil ODS-EP is useful for the LC/MS analysis.

- Superior peak shapes of both acids and bases can be obtained because of neutral bonded phase and low residual silanol groups.

- Silica gel of high-purity is used as the support material, which minimizes effects of any remaining metal ions.